



# CERTIFICATE OF ANALYSIS

## K200 Eluant for Ion-exchange Chromatography of Glyphosate and AMPA K200

45

**Product:** K200 Eluant for ion-exchange chromatography of glyphosate and AMPA  
**Part Number:** K200  
**Lot Number:** 00 501 3  
**Test Start Date:** 14 MAY 2010  
**Expiration Date:** 12 MAY 2012

**Primary Application:** Eluant for ion-exchange chromatography of glyphosate and AMPA

**Acceptance Criteria:**

1. pH =  $2.00 \pm 0.05$  at  $25 \pm 0.4$  °C
2. Elution times meet specifications
  - Glyphosate (Y/N)
  - AMPA (Y/N)
3. AMPA and Glyphosate area meet specifications (Y/N)  
 NOTE: Area ratios are affected by the hypochlorite added to GA116
4. Baseline noise ( $0 \pm 25$  mvolts) (Y/N)

**Actual Values**

2.000

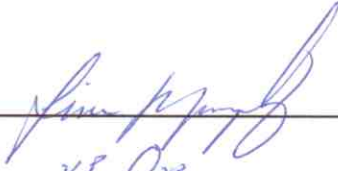
Y

Y

Y

Y

**Storage Conditions:** Dry at 8 to 25 °C

**Analysis Certified by:**  **Date:** 19 MAY 2010

VP Dir  
Title

Rev. 6, 8/11/08

**ACCEPTED**  
PICKERING LABORATORIES, INC.  
QUALITY ASSURANCE